

Manufacturing Plant: Via Benessea, 29/B 17035 - Cisano sul Neva (SV) www.narda-sts.it Tel.: +39 0182 58641 Fax: +39 0182 586400

nardait.support@narda-sts.it narda-sts@onlinepec.it



User's Manual PMM AS02 PMM AS03 PMM AS04 PMM AS05 PMM AS06 **PMM AS07** PMM AS08

ANTENNA SET

SERIAL NUMBER OF THE INSTRUMENT

You can find the Serial Number near the RF connector on both antennas. Serial Number is in the form: 0000X00000. The first four digits and the letter are the Serial Number prefix, the last five digits are

the Serial Number suffix. The prefix is the same for identical instruments, it changes only when a configuration change is made to the instrument. The suffix is different for each instrument.

Document ASEN-40313 - Copyright © NARDA 2024



NOTE:

® Names and Logo are registered trademarks of Narda Safety Test Solutions GmbH – Trade names are trademarks of the owners.

CAUTION

If the instrument is used in any other way than as described in this User's Manual, it may become unsafe.

Before using this product, the related documentation must be read with great care and fully understood to familiarize with all the safety prescriptions.

To ensure the correct use and the maximum safety level, the User shall know all the instructions and recommendations contained in this document.

WARNING

This product is a Safety Class I instrument according to IEC classification and has been designed to meet the requirements of EN61010-1 (Safety Requirements for Electrical Equipment for Measurement, Control and Laboratory Use).

In accordance with the IEC classification, the power supply of this product meets requirements Safety Class II and Installation Category II (having double insulation and able to carry out mono-phase power supply operations).


It complies with the requirements of Pollution Class II (usually only non-conductive pollution). However, occasionally it may become temporarily conductive due to condense on it.

The information contained in this document is subject to change without notice.

EXPLANATION OF ELECTRICAL AND SAFETY SYMBOLS :



You now own a high-quality instrument that will give you many years of reliable service. Nevertheless, even this product will eventually become obsolete. When that time comes, please remember that electronic equipment must be disposed of in accordance with local regulations. This product conforms to the WEEE Directive of the European Union (2002/96/EC) and belongs to Category 9 (Monitoring and Control Instruments). You can return the instrument to us free of charge for proper environment friendly disposal. You can obtain further information from your local Narda Sales Partner or by visiting our website at www.narda-sts.it .

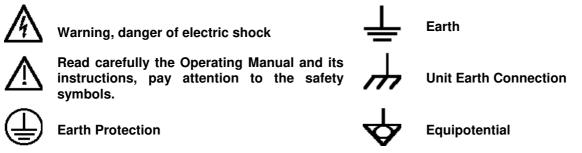

EXPLANATION OF SYMBOLS USED IN THIS DOCUMENT :



The DANGER sign draws attention to a serious risk to a person's safety, which, if not avoided, will result in death or serious injury. All the precautions must be fully understood and applied before proceeding.







The WARNING sign indicates a hazardous situation, which, if not avoided, could result in death or serious injury. All the precautions must be fully understood and applied before proceeding.

The CAUTION sign indicates a hazardous situation, which, if not avoided, could result in minor or moderate injury.

The NOTICE sign draws attention to a potential risk of damage to the apparatus or loss of data.



The NOTE sign draws attention to important information.



EC Conformity



Contents

Safety recommendations and instructions	V
EC Declaration of Conformity BC-01	
EC Declaration of Conformity BL-01	VII
EC Declaration of Conformity DR-01	VIIII
EC Declaration of Conformity LP-02, LP-03, LP-04	IX
EC Declaration of Conformity AS-02, AS-03, AS-04, AS-05, AS-06, AS-07, AS-08	Х

1 General information

Page

1.1 Introduction	1-1
1.2 Documentation.	1-1
1.3 Introduction to the PMM Antenna Set.	1-1
1.4 Standard accessories	• •
	1-2
1.4.1 PMM AS-02 Antenna Set	1-2
1.4.2 PMM AS-03 Antenna Set	1-3
1.4.3 PMM AS-04 Antenna Set	1-4
1.4.4 PMM AS-05 Antenna Set	1-5
1.4.5 PMM AS-06 Antenna Set	1-6
1.4.6 PMM AS-07 Antenna Set	1-7
1.4.7 PMM AS-08 Antenna Set	1-8
1.5 Optional accessories	1-9
1.6 PMM BC-01 Biconical Dipole Antenna	1-10
1.7 PMM BL-01 Biconical Log Periodic Dipole Array	1-11
1.8 PMM LP-02 Log Periodic Dipole Array	1-12
1.9 PMM LP-03 Log Periodic Dipole Array	1-13
1.10 PMM LP-04 Log Periodic Dipole Array	1-14
1.11 PMM DR-01 Double Ridged horn antenna	1-15
1.12 BC-01 Main Specifications	1-16
1.13 BL-01 Main Specifications	1-19
1.14 LP-02 Main Specifications	1-21
1.15 LP-03 Main Specifications	1-25
1.16 LP-04 Main Specifications	1-27
1.17 DR-01 Main Specifications	1-29
1.18 TR-01 Main Specifications	1-31
1.19 RF Cable 5m Main Specifications	1-32

2 Mounting Instructions

2 Mounting Instructions	Page
2.1 Introduction	2-1
2.2 Initial inspection	2-1
2.3 Environment	2-1
2.4 Return for service	2-1
2.5 Equipment cleaning	2-1
2.6 PMM BC-01 Biconical Dipole Array	2-2
2.7 PMM BL-01 Biconical Log Periodic Dipole Array	2-3
2.8 PMM LP-02 Log Periodic Dipole Array	2-8
2.9 PMM LP-03 Log Periodic Dipole Array	2-9
2.10 PMM LP-04 Log Periodic Dipole Array	2-11

3 Radiated Emission and Immunity testing 3.1 Radiated emission testing	Page 3-1
3.1.1 The receiver antenna	3-1
3.1.2 The interconnecting cable	3-1
3.1.3 The preamplifier 3.1.4 The preamplifier interconnecting cable	3-1 3-1
3.1.5 The meter receiver	3-2
3.2 Radiated immunity testing	3-3
3.2.1 The signal generator 3.2.2 The power amplifier	3-3 3-3
3.2.3 The transmit antenna 3.2.4 The field strength meter	3-3 3-3
3.3 Environmental testing.	3-5 3-5



Figures

Figure		Pa
1-1	PMM AS-02 kit	1-2
1-2	PMM AS-03 kit	1-:
1-3	PMM AS-04 kit	1-
1-4	PMM AS-05 kit	1-
1-5	PMM AS-06 kit	1-
1-6	PMM AS-07 kit	1-
1-7	PMM AS-08 kit	1-
1-8	PMM BC-01	1-
1-9	PMM BL-01	1-
1-10	PMM LP-02	1-
1-11	PMM LP-03	1-
1-12	PMM LP-04	1-
1-13	PMM DR-01	1-
1-14	Typical BC-01 antenna factor @ 3 m	1-
1-15	Typical BC-01 antenna factor @ 10 m	1-
1-16	Typical BL-01 antenna factor	1-
1-17	Typical BL-01 VSWR	1-3
1-18	Typical LP-02 antenna factor @ 3 m	1-3
1-19	Typical LP-02 antenna factor @ 10 m	1-3
1-20	Typical LP-02 VSWR	1-3
1-21	Typical LP-03 Antenna Factor	1-:
1-22	Typical LP-03 Gain	1-:
1-23	Typical LP-03 VSWR	1-:
1-24	Typical LP-04 Antenna Factor	1-:
1-25	Typical LP-04 VSWR	1-:
1-26	Typical DR-01Antenna Factor	1-:
1-27	Typical DR-01VSWR	1-3
1-28	Mounting head with center column	1-3
1-29	Adjustable joint	1-:
1-30	Typical RF Cable/5 insertion loss	1-:
2-1	PMM BC-01 with TR-01	2-
2-2	PMM BL-01 with TR-01	2-
2-3	PMM LP-02 with TR-01	2-
2-4	PMM LP-03 with TR-01	2-
2-5	PMM LP-04 with TR-01	2-
3-1	Radiated emission test setup	3-
3-2	Radiated immunity test setup	3-4
0-2		

Tables

Table		Page
1-1	PMM BC-01 Biconical Dipole Specifications	1-16
1-2	PMM BL-01 Biconical Dipole Specifications	1-19
1-3	PMM LP-02 Log Periodic Dipole Array Specifications	1-21
1-4	PMM LP-03 Log Periodic Dipole Array Specifications	1-25
1-5	PMM LP-04 Log Periodic Dipole Array Specifications	1-27
1-6	PMM DR-01 Double ridged Antenna Specifications	1-29
1-7	PMM TR-01 Wooden Tripod Specifications	1-31
1-8	PMM RF Cable / 5 Specifications	1-32

IV



WARNING SAFETY RECOMMENDATIONS AND INSTRUCTIONS

This product has been designed, produced and tested in Italy, and it left the factory in conditions fully complying with the current safety standards. To maintain it in safe conditions and ensure correct use, these general instructions must be fully understood and applied before the product is used.

- When the device must be connected permanently, first provide effective grounding;
- If the device must be connected to other equipment or accessories, make sure they are all safely grounded;
- Any interruption or loosening of the ground wire or of a connecting power cable, inside or outside the device, will cause a potential risk for the safety of the personnel;
- Ground connections must not be interrupted intentionally;
- To prevent the possible danger of electrocution, do not remove any covers, panels or guards installed on the device, and refer only to NARDA Service Centers if maintenance should be necessary;
- Follow the safety regulations and any additional instructions in this manual to prevent accidents and damages.



In accordo alla Decisione 768/2008/EC, conforme alle direttive EMC 2014/30/UE, Bassa Tensione 2014/35/UE e RoHS 2011/65/UE, ed anche alle norme ISO/IEC 17050-1 e 17050-2. *In accordance with the Decision 768/2008/EC, compliant to the Directives EMC 2014/30/UE, Low Voltage 2014/35/UE and* RoHS 2011/65/EU, *also compliant to the ISO/IEC standard 17050-1 and 17050-2*

ll costruttore The manufacturer	narda Safety Test Solutions S.r.l. Socio Unico		
Indirizzo <i>Address</i>	Via Benessea, 29 / B		
	I-17035 Cisano sul Neva (SV) - Italy		
	enti norme europee armonizzate, applicate con esito positivo: ng harmonized European Standards, successfully applied:		
Sicurezza: <i>Safety:</i>	EN 61010-1 (2010)		
	pria responsabilità, che il prodotto: ole responsibility, that the product: ANTENNA BICONICA		
Description	BICONICAL DIPOLE ANTENNA		
Modello <i>Model</i>	PMM BC-01		
	iti essenziali delle seguenti Direttive: ssential requirements of the following Directives:		
Bassa Tensione <i>Low Voltage</i>	2014/35/EU		
RoHS <i>RoHS</i>	2011/65/EU		
Cisano sul Neva, 14 March 2024 Egon Stocca			

General Manager

VI



In accordo alla Decisione 768/2008/EC, conforme alle direttive EMC 2014/30/UE, Bassa Tensione 2014/35/UE e RoHS 2011/65/UE, ed anche alle norme ISO/IEC 17050-1 e 17050-2. In accordance with the Decision 768/2008/EC, compliant to the Directives EMC 2014/30/UE, Low Voltage 2014/35/UE and RoHS 2011/65/EU, also compliant to the ISO/IEC standard 17050-1 and 17050-2

Il costruttore The manufacturer	narda Safety Test Solutions S.r.I. Socio Unico		
Indirizzo <i>Address</i>	Via Benessea, 2	9 / B	
	I-17035 Cisano s	sul Neva (SV) - Italy	
		armonizzate, applicate con esito positivo: pean Standards, successfully applied:	
Sicurezza: <i>Safety:</i>	EN 61010-1 (2010)		
dichiara, sotto la pro declares, under its s			
Descrizione Description	ANTENNA BICONICA LOG-PERIODICA BICONICAL LOG PERIODIC DIPOLE ARRAY ANTENNA		
Modello <i>Model</i>	PMM BL-01		
	iti essenziali delle se ssential requirement	eguenti Direttive: s of the following Directives:	
Bassa Tensione Low Voltage	2014/35	5/EU	
RoHS <i>RoHS</i>	2011/65	5/EU	
Cisano sul Neva, 14 March 2024		Egon Stocca	
		General Manager	
		Hef	

VII



In accordo alla Decisione 768/2008/EC, conforme alle direttive EMC 2014/30/UE, Bassa Tensione 2014/35/UE e RoHS 2011/65/UE, ed anche alle norme ISO/IEC 17050-1 e 17050-2. *In accordance with the Decision 768/2008/EC, compliant to the Directives EMC 2014/30/UE, Low Voltage 2014/35/UE and* RoHS 2011/65/EU, *also compliant to the ISO/IEC standard 17050-1 and 17050-2*

ll costruttore The manufacturer	narda Safety Test Solutions S.r.I. Socio Unico			
Indirizzo <i>Address</i>	Via Benessea, 2	9 / B		
	I-17035 Cisano	sul Neva (SV) - Italy		
		armonizzate, applicate con esito positivo: pean Standards, successfully applied:		
Sicurezza: <i>Safety:</i>				
	opria responsabilità, sole responsibility, th			
Descrizione Description	ANTENNA A TROMBA DOUBLE RIDGED HORN ANTENNA			
Modello <i>Model</i>	PMM DR-01			
	isiti essenziali delle se essential requirement	eguenti Direttive: s of the following Directives:		
Bassa Tensione <i>Low Voltage</i>	_2014/3	5/EU		
RoHS <i>RoHS</i>	2011/65	5/EU		
Cisano sul Neva, 1	4 March 2024	Egon Stocca		
		General Manager		

VIII



In accordo alla Decisione 768/2008/EC, conforme alle direttive EMC 2014/30/UE, Bassa Tensione 2014/35/UE e RoHS 2011/65/UE, ed anche alle norme ISO/IEC 17050-1 e 17050-2. *In accordance with the Decision 768/2008/EC, compliant to the Directives EMC 2014/30/UE, Low Voltage 2014/35/UE and* RoHS 2011/65/EU, *also compliant to the ISO/IEC standard 17050-1 and 17050-2*

Il costruttore The manufacturer	narda Safety Test Solutions S.r.I. Socio Unico			
Indirizzo <i>Address</i>	Via Benessea, 2	Via Benessea, 29 / B		
	I-17035 Cisano	sul Neva (SV) - Italy		
		e armonizzate, applicate con esito positivo: opean Standards, successfully applied:		
Sicurezza: <i>Safety:</i>	EN 61010-1 (2010))		
	ropria responsabilità, <i>sole responsibility, tl</i>			
Descrizione Description		ANTENNA LOG-PERIODICA LOG PERIODIC DIPOLE ARRAY ANTENNA		
Modello <i>Model</i>	PMM LP-02, LP-03, LP-04			
	isiti essenziali delle s essential requirement	eguenti Direttive: ts of the following Directives:		
Bassa Tensione <i>Low Voltage</i>	_2014/3	5/EU		
RoHS <i>RoHS</i>	2011/6	5/EU		
Cisano sul Neva, 14 March 2024		Egon Stocca		
		General Manager		
		$\bigcirc \rho \land \land$		

hef

IX



In accordo alla Decisione 768/2008/EC, conforme alle direttive EMC 2014/30/UE, Bassa Tensione 2014/35/UE e RoHS 2011/65/UE, ed anche alle norme ISO/IEC 17050-1 e 17050-2. *In accordance with the Decision 768/2008/EC, compliant to the Directives EMC 2014/30/UE, Low Voltage 2014/35/UE and* RoHS 2011/65/EU, *also compliant to the ISO/IEC standard 17050-1 and 17050-2*

ll costruttore The manufacturer	narda Safety Test Solutions S.r.I. Socio Unico				
Indirizzo <i>Address</i>	Via Benessea, 29 / B				
	I-17035 Cisano sul Neva (SV) - Italy				
	uenti norme europee armonizzate, applicate con esito positivo: ing harmonized European Standards, successfully applied:				
Sicurezza: <i>Safety:</i>	EN 61010-1 (2010)				
	opria responsabilità, che il prodotto: sole responsibility, that the product:				
Descrizione Description	SISTEMA DI ANTENNA ANTENNA SET				
Modello <i>Model</i>	PMM AS-02, AS-03, AS-04, AS-05, AS-06, AS-07, AS-08				
	siti essenziali delle seguenti Direttive: essential requirements of the following Directives:				
Bassa Tensione <i>Low Voltage</i>	2014/35/EU				
RoHS <i>RoHS</i>	2011/65/EU				
Cisano sul Neva, 14	4 March 2024 Egon Stocca				

Egon Stocca General Manager

Х



1 – General Information

This manual is a guide to the installation and use of the PMM AS-02, AS-1.1 Introduction 03, AS-04, AS-05, AS-06, AS-07 and AS-08 Antenna Set. Main information about the radiated emission and immunity testing are also explained. **1.2 Documentation**

Enclosed with this manual are:

- a service questionnaire to send back to NARDA if equipment service is required.
- an accessories check list to verify all accessories enclosed in the packaging.
- With a compact size, easy mounting set and polarization change, light 1.3 Introduction to the weight and broadband frequency range the Antenna Set series is the ideal PMM Antenna Set solution for automated measurements in the 30 MHz to 18 GHz frequency range.

The PMM AS-02 covers from 30 MHz to 3 GHz, the AS-03/AS-04/AS-07 from 30 MHz to 6 GHz and the AS-05/AS-06/AS-08 from 30 MHz to 18 GHz. Common applications include measurements to EN 55022 emission and CEI IEC 61000-4-3 immunity testing specifications.

The PMM AS-02 is composed of a PMM BC-01 Bi-Conical Dipole and PMM LP-02 Log Periodic Dipole Array.

The PMM AS-03 and AS-06 include a PMM BC-01 Bi-Conical Dipole, PMM LP-02 Log Periodic Dipole Array, PMM LP-03 Log Periodic Dipole Array and PMM DR-01 Double Ridged Horn Antenna (for PMM AS-06 only).

The PMM AS-04 and AS-05 are composed of a PMM BC-01 Bi-Conical Dipole, PMM LP-04 Log Periodic Dipole Array and PMM DR-01 Double Ridged Horn Antenna (for PMM AS-05 only).

The PMM AS-07 and AS-08 include a BL-01 Bi-Conical Log Periodic Dipole Array and PMM DR-01 Double Ridged Horn Antenna (for PMM AS-08 only).

The supplied tripod PMM TR-01 is highly recommended: the tripod stand is made by hard wood assuring the needed rigidity when holding the antenna. the adjustable joint allows easy to mount and antenna polarization change operations.

Document ASEN-40313 - © NARDA 2024

General information 1**-1**



1.4 Standard Accessories

1.4.1 PMM AS-02 (30 MHz – 3 GHz) The PMM Antenna Set are kits that include multiple units and standard accessories; they are described in the following paragraphs.

The PMM AS-02 Antenna Set includes the following standard accessories:

- BC-01 Bi-Conical Dipole Antenna
- LP-02 Log Periodic Dipole Array
- TR-01 Wooden tripod with extension and adjustable joint
- RF Cable/5 RF cable (5m long)
- CC-01 Soft Carrying case
- Antennas Calibration Reports (one for each antenna unit)
- User's manual



Fig. 1-1 PMM AS-02 kit

1-2 General information



1.4.2 PMM AS-03

(30 MHz – 6 GHz)

The PMM AS-03 Antenna Set includes the following standard accessories:

- BC-01 Bi-Conical Dipole Antenna
- LP-02 Log Periodic Dipole Array
- LP-03 Log Periodic Dipole Array
- TR-01 Wooden tripod with extension and adjustable joint
- RF Cable/5 RF cable (5m long)
- N(f)-N(f) adapter
- CC-01 Soft Carrying case
- CC-03 Soft Carrying case
- Support for LP-03
- Antennas Calibration Reports (one for each antenna unit)
- User's manual



Fig. 1-2 PMM AS-03 kit



1.4.3 PMM AS-04 (30 MHz – 6 GHz) The PMM AS-04 Antenna Set includes the following standard accessories:

- BC-01 Bi-Conical Dipole Antenna
- LP-04 Log Periodic Dipole Array
- CC-01 Soft Carrying case
- TR-01 Wooden tripod with extension and adjustable joint
- RF Cable/5 RF cable (5m long)
- Antennas Calibration Reports (one for each antenna unit)
- User's manual



Fig. 1-3 PMM AS-04 kit



1.4.4 PMM AS-05

(30 MHz – 18 GHz)

The PMM AS-05 Antenna Set includes the following standard accessories:

- BC-01 Bi-Conical Dipole Antenna
- LP-04 Log Periodic Dipole Array
- DR-01 Double Ridged Horn Antenna
- TR-01 Wooden tripod with extension and adjustable joint
- Antenna Support kit for DR-01
- CC-01 Soft Carrying case
- 170/30N Rigid Carrying case (for DR-01)
- RF Cable/5 RF cable (5m long)
- Antennas Calibration Reports (one for each antenna unit)
- User's manual



Fig. 1-4 PMM AS-05 kit



1.4.5 PMM AS-06

(30 MHz – 18 GHz)

The PMM AS-06 Antenna Set includes the following standard accessories:

- BC-01 Bi-Conical Dipole Antenna
- LP-02 Log Periodic Dipole Array
- LP-03 Log Periodic Dipole Array
- DR-01 Double Ridged Horn Antenna
- TR-01 Wooden tripod with extension and adjustable joint
- Support for LP-03
- Antenna Support kit for DR-01
- CC-01 Soft Carrying case
- CC-03 Soft Carrying case
- 170/30N Rigid Carrying case (for DR-01)
- RF Cable/5 RF cable (5m long)
- N(f)-N(f) adapter
- Antennas Calibration Reports (one for each antenna unit)
- User's manual



Fig. 1-5 PMM AS-06 kit



1.4.6 PMM AS-07

(30 MHz – 6 GHz)

The PMM AS-07 Antenna Set includes the following standard accessories:

- BL-01 Bi-Conical Log Periodic Antenna
- CC-02 Soft Carrying case
- TR-01 Wooden tripod with extension and adjustable joint
- RF Cable/5 RF cable (5m long)
- BL-01 Calibration Report
- User's manual



Fig. 1-6 PMM AS-07 kit



1.4.7 PMM AS-08 (30 MHz – 18 GHz) The PMM AS-08 Antenna Set includes the following standard accessories:

- BL-01 Bi-Conical Log Periodic Antenna
- DR-01 Double Ridged Horn Antenna
- TR-01 Wooden tripod with extension and adjustable joint
- Antenna Support kit for DR-01
- CC-02 Soft Carrying case
- 170/30N Rigid Carrying case (for DR-01)
- RF Cable/5 RF cable (5m long)
- Antennas Calibration Reports (one for each antenna unit)
- User's manual



Fig. 1-7 PMM AS-08 kit



1.5 Optional

Accessories

The following accessories can be ordered separately:

- BC-01 Bi-Conical Dipole Antenna
- BC-01/TC Bi-Conical Dipole Antenna (typical calibration)
- BL-01 Bi-Conical Log-periodic Antenna
- BL-01/TC Bi-Conical Log-periodic Antenna (typical calibration)
- LP-02 Log Periodic Dipole Array
- LP-02/TC Log Periodic Dipole Array (typical calibration)
- LP-03 Log Periodic Dipole Array
- LP-03/TC Log Periodic Dipole Array (typical calibration)
- LP-04 Log Periodic Dipole Array
- LP-04/TC Log Periodic Dipole Array (typical calibration)
- DR-01 Double Ridged Horn Antenna
- PMM TR-01 Wooden tripod;
- Support for LP-03
- Antenna Support kit for DR-01
- CC-01 Soft Carrying case
- CC-02 Soft Carrying case
- CC-03 Soft Carrying case
- 170/30N Rigid Carrying case (for DR-01)
- RF Cable/5 RF cable (5 m long)
- N(f)-N(f) adapter
- AMK-01 Antenna Mounting Kit for AS-02/AS-03/AS-04/AS-05/AS-06
- AMK-02 Antenna Mounting Kit for AS-07/AS-08



For some models, it is available a "typical calibration". For these units, the calibration report contains typical values that are generally very close to the actual ones.



1.6 PMM BC-01 Bi-Conical Dipole Antenna

The PMM BC-01 Bi-Conical Dipole is a compact size and time saving alternative to the classical dipole antenna in the range 30 - 200 MHz; the tedious manual adjustment at each frequency of the classical dipole elements can be avoided using the compact size and broadband frequency range characteristics of the PMM AS-02, AS-03, AS-04, AS-05 and AS-06 kit.



Fig. 1-8 PMM BC-01

The PMM BC-01 can be ordered separately and, in this case, includes:

- Soft Tubular Case;
- Calibration Report;
- User's manual


- **TR-01 set** (includes: TR01 60-180 cm wooden column extendable tripod, antenna mounting adapter to change polarization, soft carrying case)
- **RF cable** 5 meter/6 GHz/N(m)-N(m)
- **AMK-01** Antenna Mounting kit



1.7 PMM BL-01 Bi-Conical Log-periodic Antenna A versatile PMM BL-01 Bi-Conical Log Periodic Dipole Array covers the full range 30 MHz to 6 GHz without changing antennas, even if such a solutions is mostly more expensive and the antenna size is bigger.

Its ideal companion is the EMI Receiver Unit PMM 9060, which can be easily mounted on the antenna by optional accessory AMK-02.

On the PMM AS-07 kit is available the BL-01 antenna with TR-01 set and RF cable 5m.

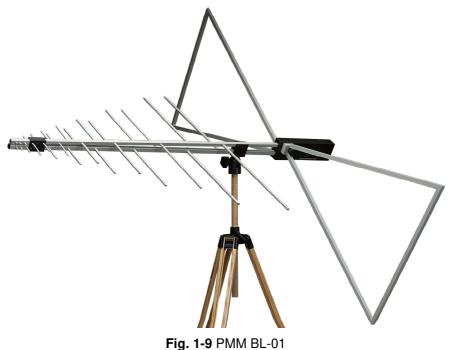

On the PMM AS-08 kit is also available a double ridged horn antenna for measurements above 6 GHz.

The PMM BL-01 can be ordered separately and, in this case, includes:

- CC-02 Soft Carrying Case;
- Calibration Report;
- User's manual.

- **TR-01 set** (includes: TR01 60-180 cm wooden column extendable tripod, antenna mounting adapter to change polarization, soft carrying case)
- **RF cable** 5 meter/6 GHz/N(m)-N(m)
- AMK-02 Antenna Mounting kit



1.8 PMM LP-02 Log Periodic Dipole Array The PMM LP-02 Log Periodic Dipole Array obtain a broadband excellent VSWR characteristics thanks to its accurate design of the feed and elements positioning on the boom, the constant antenna gain yields an antenna factor which varies linearly with frequency in the range 200 MHz to 3 GHz.



Fig. 1-10 PMM LP-02

The PMM LP-02 can be ordered separately and, in this case, includes:

- CC-01 Soft carrying case;
- Calibration Report;
- User's manual

- **TR-01 set** (includes: TR01 60-180 cm wooden column extendable tripod, antenna mounting adapter to change polarization, soft carrying case)
- **RF cable** 5 meter/6 GHz/N(m)-N(m)
- AMK-01 Antenna Mounting kit



1.9 PMM LP-03 Log Periodic Dipole Array The PMM LP-03 Log Periodic Dipole Array obtain a broadband excellent VSWR characteristics thanks to its accurate design of the feed and elements positioning on the boom, the constant antenna gain yields an antenna factor which varies linearly with frequency in the range 0.8 to 6 GHz.

The PMM LP-03 has been developed and specified mainly as accessory of the 6 GHz receivers 9060. The LP-03 can be also offered as a general purpose antenna for both EMC and other industrial applications, alone or in an antenna kit (PMM AS-03).

The booms and the elements are made of aluminium Alodyne coated and painted; the holding pipe is made of stainless steel; the antenna is composed by a total of 28 elements.

The LP-03 combines small size with high manufacturing and calibration standards, making it perfectly suitable for portable applications and in anechoic chambers.

The tripod PMM TR-01 is highly recommended; the tripod stand is made by hard wood assuring the needed rigidity when holding the antenna, the adjustable joint allows easy to mount and antenna polarization change operations.



Fig. 1-11 PMM LP-03

The PMM LP-03 can be ordered separately and, in this case, includes:

- Support for LP-03;
- CC-03 Soft Carrying Case;
- Nf to Nf Adapter
- n°2 3MAx16mm screws
- Calibration Report;
- User's manual

- **TR-01 set** (includes: TR01 60-180 cm wooden column extendable tripod, antenna mounting adapter to change polarization, soft carrying case)
- **RF cable** 5 meter/6 GHz/N(m)-N(m)



1.10 PMM LP-04 Log Periodic Dipole Array The PMM LP-04 Log Periodic Dipole Array obtain a broadband excellent VSWR characteristics thanks to its accurate design of the feed and elements positioning on the boom, the constant antenna gain yields an antenna factor which varies linearly with frequency in the range 200 MHz to 6 GHz.



Fig. 1-12 PMM LP-04

The PMM LP-04 can be ordered separately and, in this case, includes:

- CC-01 Soft carrying case;
- Calibration Report;
- User's manual

- **TR-01 set** (includes: TR01 60-180 cm wooden column extendable tripod, antenna mounting adapter to change polarization, soft carrying case)
- **RF cable** 5 meter/6 GHz/N(m)-N(m)
- AMK-01 Antenna Mounting kit



1.11 PMM DR-01 Double Ridged horn antenna

The PMM DR-01 Double Ridged is a compact Horn Antenna with a broadband response in the frequency range of 6 GHz - 18 GHz. It is designed for direct connection - without cable or adapters to the 18 GHz receiver PMM 9180.

The DR-01 can be connected to any other RF equipment: small size with high manufacturing and calibration standards make it perfectly suitable for portable applications and in anechoic chambers.

Each unit is individually calibrated before shipment; the test data are supplied with the antenna.

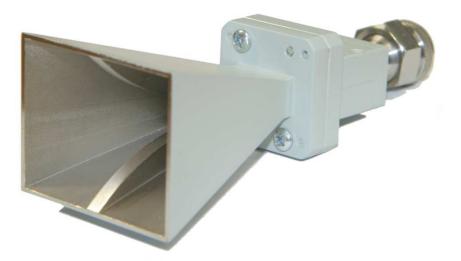


Fig. 1-13 PMM DR-01

The supplied tripod PMM TR-01 is recommended; the tripod stand is made by hard wood assuring the stability needed for holding antenna and receiver PMM 9180; the adjustable joint allows for easy antenna mounting and polarization changing.

The PMM DR-01 can be ordered separately and, in this case, includes:

- 170/30N Rigid Carrying Case;
- Nf to Nf Adapter
- Antenna Support kit;
- Calibration Report;
- User's manual



1.12 BC-01 Main Specifications

The following Table list the BC-01 Antenna performance specifications.

TABLE 1-1 PMM BC-01 Biconical Dipole Specifications		
Electrical characteristics	Performance Limits	
Frequency range	30 to 200 MHz	
Impedance	50 Ω nominal	
Gain	-15 +2 dBi typical	
Antenna Factor	8 to 14 dB/m typical	
Construction	Aluminium	
Max input power	100 W	
Connector	N-female	
Dimensions (L x H x W)	65 x 65 x 137 cm	
Weight	1,8 kg	
Colour	RAL 7035	



3 m Typical Antenna Factor

Calibration Distance & Polarisation Receiving Antenna Height Transmitting Antenna Height 3,0 m Horizontal 1-4 m 1 m

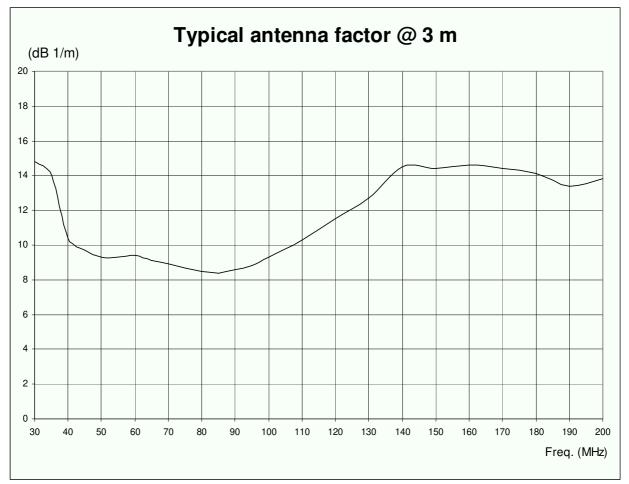


Fig. 1-14 Typical BC-01 antenna factor @ 3 m



10 m Typical Antenna Factor

Calibration Distance & Polarisation Receiving Antenna Height Transmitting Antenna Height 10,0 m Horizontal 1-4 m 1 m

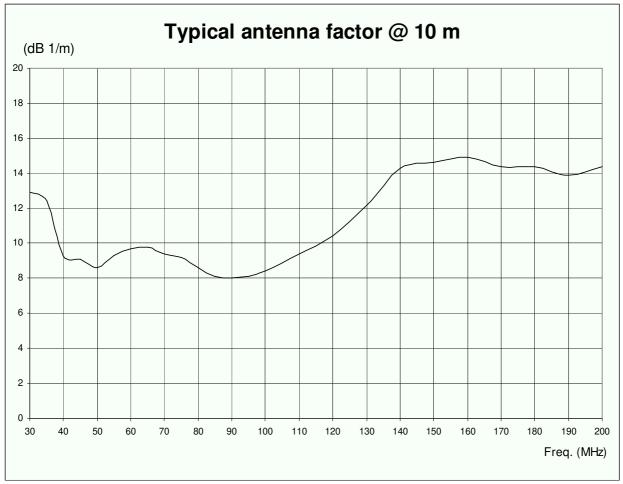


Fig. 1-15 Typical BC-01 antenna factor @ 10 m



1.13 BL-01 Main

The following Table list the BL-01 Antenna performance specifications.

Specifications

TABLE 1-2 PMM BL-01 Biconical Log-periodic Dipole Specifications		
Electrical characteristics	Performance Limits	
Frequency range	30 MHz to 6 GHz	
Impedance	50 Ω nominal	
Gain	-9 to +5 dBi typical	
Antenna factor	8 to 45 dB/m typical	
VSWR 30 MHz 60 to 120 MHz 120 to 170 MHz 170 MHz to 6 GHz	< 16:1 typical < 4:1 typical < 2:1 typical < 1.5:1 typical	
Construction	Aluminium	
Max input power	100 W up to 1 GHz 50 W up to 3 GHz	
Connector	N female	
Dimensions (L x H x W)	145 x 61 x 157 cm	
Weight	5,5 kg	
Colour	RAL 7035	


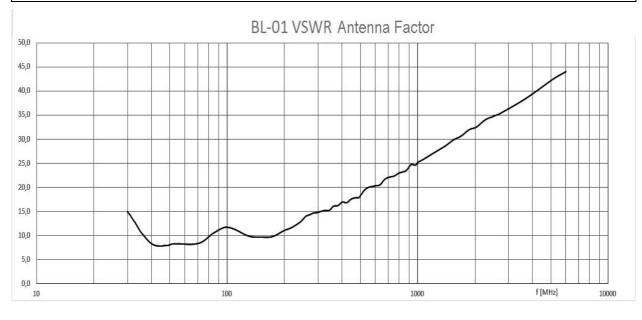


Fig. 1-16 Typical BL-01 antenna factor





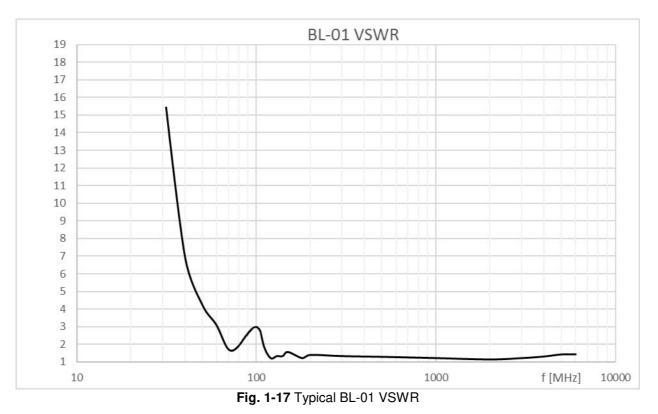

1.14 LP-02 Main Specifications

The following Table list the LP-02 Antenna performance specifications.

TABLE 1-3 PMM LP-02 Log Periodic Dipole Array Specifications		
Electrical characteristics	Performance Limits	
Frequency range	200 MHz - 3 GHz	
Impedance	50 Ω nominal	
Gain	6 dBi typical	
Antenna Factor	13 to 36 dB/m typical	
VSWR	< 2:1 (1,2:1 typ.)	
Construction	Aluminium	
Max input power	100 W up to 1 GHz 50 W up to 3 GHz	
Connector	N-female	
Dimensions (L x H x W)	70 x 10 x 86 cm	
Weight	1,1 kg	
Colour	RAL 7035	



3 m Typical Antenna Factor

Calibration Distance & Polarisation	3,0 m	Horizontal
Receiving Antenna Height	1-4 m	
Transmitting Antenna Height	1 m	

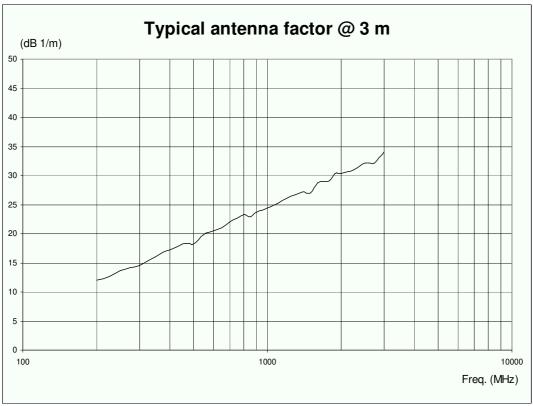


Fig. 1-18 Typical LP-02 antenna factor @ 3 m



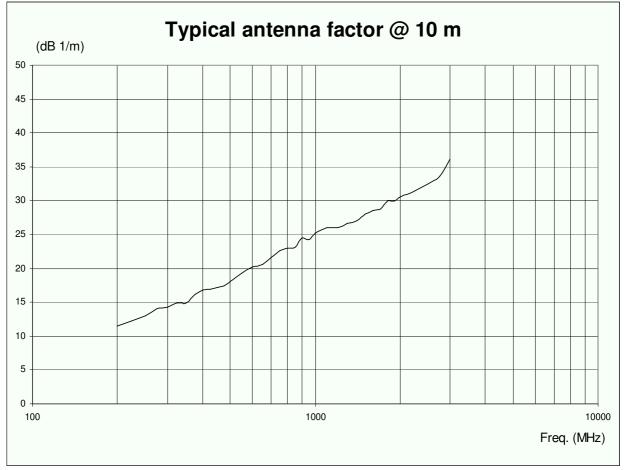


Fig. 1-19 Typical LP-02 antenna factor @ 10 m



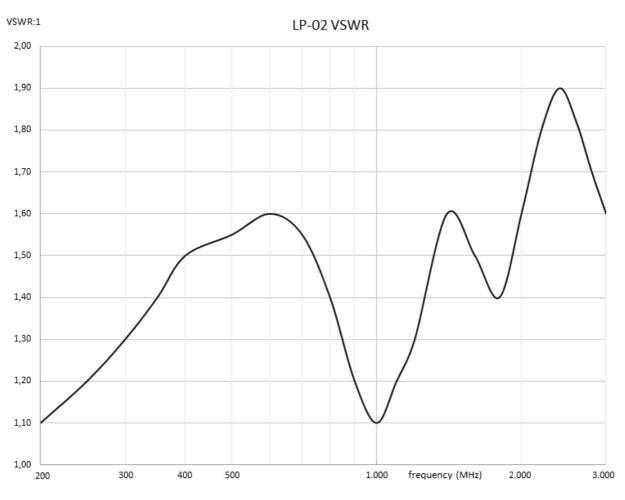


Fig. 1-20 Typical LP-02 VSWR

1.15 LP-03 Main Specifications

The following Table list the LP-03 Antenna performance specifications.

TABLE 1-4 PMM LP-03 Log Periodic Dipole Array Specifications Electrical characteristics Performance Limits		
Frequency range	800 MHz to 6 GHz	
Impedance	50 Ω nominal	
-		
Gain	6 dBi typical	
Antenna Factor	23 to 40 dB/m typical	
VSWR	< 1,7:1 typical	
Construction	Aluminium	
Max input power	75 W	
Connector	Type N-male (LP-03)	
Dimensions (L x H x W)	32,5 x 8,1 x 18,7 cm	
Weight	0,25 kg	
Colour	RAL 7035	
1		

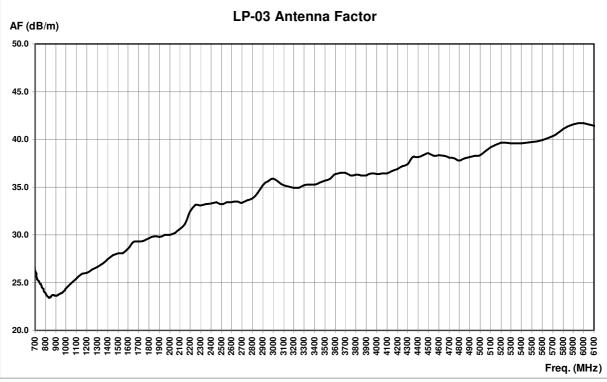


Fig. 1-21 Typical LP-03 antenna factor



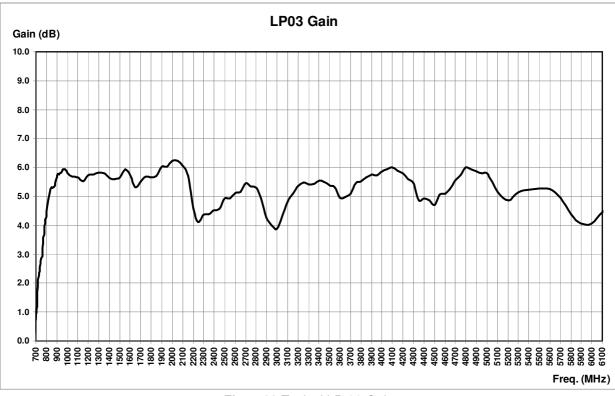


Fig. 1-22 Typical LP-03 Gain


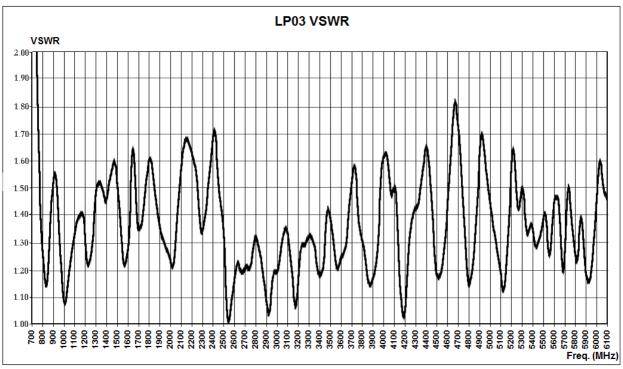


Fig. 1-23 Typical LP-03 VSWR

1.16 LP-04 Main Specifications

The following Table list the LP-04 Antenna performance specifications.

TABLE 1-5 PMM LP-04 Log Periodic Dipole Array Specifications **Electrical characteristics Performance Limits Frequency range** 200 MHz - 6 GHz Impedance 50 Ω nominal Gain 6 dBi typical **Antenna Factor** 12 to 40 dB/m typical VSWR < 1,8:1 typical Construction Aluminium 100 W Max input power Connector Type N-female Dimensions (L x H x W) 78 x 10 x 75 cm Weight 1,1 kg RAL 7035 Colour

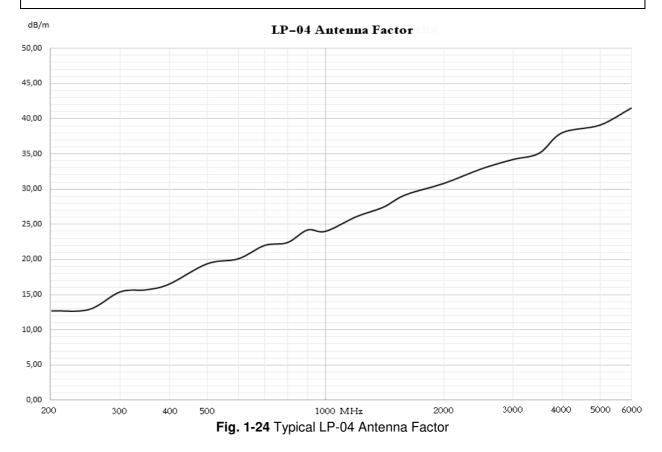

General information 1-27



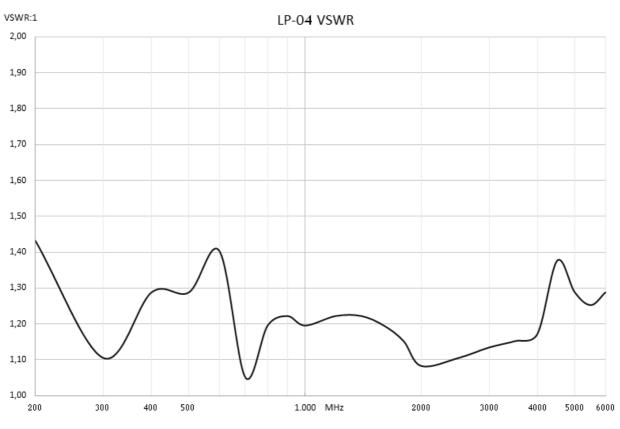


Fig. 1-25 Typical LP-04 VSWR


1.17 DR-01 Main

The following Table list the DR-01 Antenna performance specifications.

Specifications

TABLE 1-6 PMM DR-01 Double ridged Antenna Specifications			
Electrical characteristics	Performance Limits		
Frequency range	6 to 18 GHz		
Impedance	50 Ω nominal		
Gain	9 to 16 dBi		
Antenna Factor	36 to 41 dB/m		
VSWR	< 2:1 (1,8:1 typical)		
Beam width 3dB @ 12 GHz	E-plane 33° H-plane 38°		
Max input power	150 W		
Connector	N-male		
Dimensions (W x H x D)	55 x 44 x 137 mm		
Weight	0,25 kg		
Colour	RAL 7035		

Typical Antenna Factor PMM DR-01

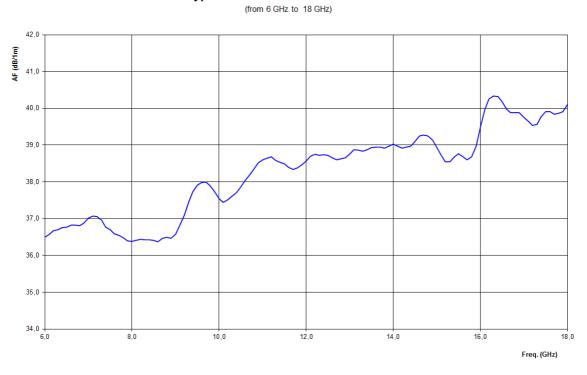





General information



Typical VSWR PMM DR-01

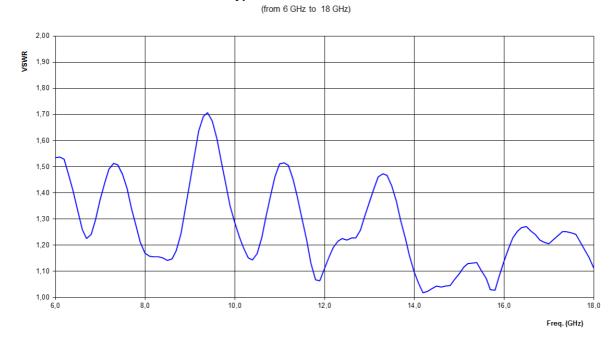





1.18 TR-01 Main Specifications

The following Table list the TR-01 Antenna performance specifications.

TABLE 1-7 PMM TR-01 Wooden tripod with extension and adjustable joint Specifications Characteristics Performance Limits

•	legs	3 legs x 3 sections extensible	
•	transportation width:	76 x 12 x 12 cm	
•	minimum height:	60 cm	
•	maximum height:	180 cm	
•	weight	2,8 kg	
•	load capacity:	10 kg	



Fig. 1-28 Mounting head with center column



Fig. 1-29 Adjustable joint

- Height: 7 cm
- Weight: 180 g
- Load capacity: 10 kg

The adjustable joint allows to easily mount the antennas on the center column of the tripod and to change the antenna polarization from horizontal to vertical or vice versa. It is possible to adjust legs spread at tree different angles, the adjustment is made rotating the knurled locking adjuster by selecting the corresponding marker on the knurled locking adjuster:

- 20° spread : knurled locking adjuster white mark;
- 45° spread : knurled locking adjuster red mark;
- variable spread : knurled locking adjuster unmarked.

The central mast can be adjusted and fixed with the clamping lever.




General information 1

1**-31**



1.19 RF Cable 5 m
Main SpecificationsThe following Table list the TR-01 Antenna performance specifications.

Electrical characteristics	Performance Limits	Performance Limits				
Connectors	N-Male					
Max Power input	300 W up to 200 MHz 100 W up to 6 GHz					
Length	5 m					
Weight	850 g					

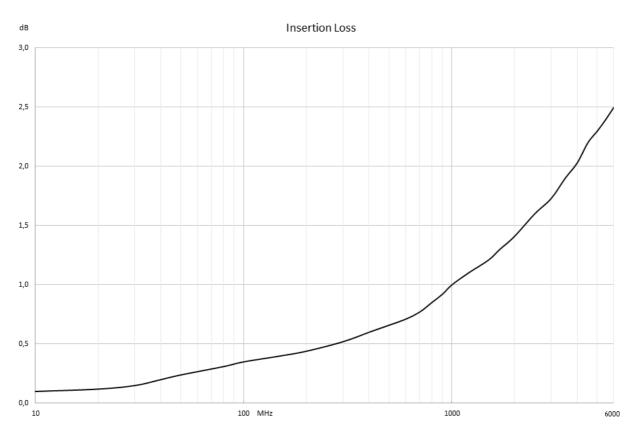





2 – Mounting Instructions

2.1 Introduction	This section provides the information needed to install and use your PMM AS-02, AS-03, AS-04, AS-05, AS-06, AS-07 and AS-08 Antenna set. Included are information pertinent to initial inspection, interconnection, environment, mechanical mounting, cleaning, storage and shipment.
2.2 Initial inspection	Inspect the shipping container for damage.
NOTICE	If the shipping container or cushion material is damaged, it should be kept until the contents of the shipment have been checked for completeness and the antennas have been checked mechanically and electrically. Verify the accessories availability in the shipping referring to the accessories check list enclosed. Notify any damage to the carrier personnel as well as the NARDA Representative.
2.3 Environment	The PMM AS-02/AS-03/AS-04/AS-05/AS-06/AS-07/AS-08 Antennas are constructed of lightweight corrosion-resistant aluminum or stainless steel, providing years of indoor and outdoor service.
2.4 Return for service	If the Antenna Set should be returned to NARDA for service, please complete the service questionnaire enclosed with the Users Manual and attach it to the instrument. To minimize the repair time, be as specific as possible when describing the failure. If possible, reuse of the original packaging to ship the equipment is preferable. In case other package should be used, ensure to wrap the instrument in heavy paper or plastic. Use a strong shipping container and use enough shock absorbing material around all sides of the equipment to provide a firm cushion and prevent movement in the container. Seal the shipping container FRAGILE to encourage careful handling.
2.5 Equipment cleaning	Use a clean, dry, non abrasive cloth for equipment cleaning.
NOTICE	To clean the wooden tripod do not use any solvent, thinner, turpentine, acid, acetone or similar matter to avoid damage to it.



2.6 PMM BC-01 Biconical Dipole Array

Screw the radiating elements on the conical fastening of the BICONICAL Antenna, the radiating elements are all of equal length.



Unscrew the knob without to loose it completely.



Insert the tripod joint on the adjustable joint.



Change the antenna polarization from horizontal to vertical or vice versa and tighten the knob completely.

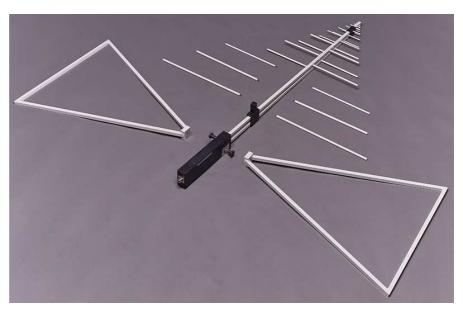


Fig. 2-1 PMM BC-01 with TR-01




2.7 PMM BL-01 Biconical Log Periodic Dipole Array

Unpacking the BL-01 antenna from the CC-02 Soft Carrying case



Assembly the BL-01 antenna starting from two shorter cylindrical dipole (299mm length) to the boom

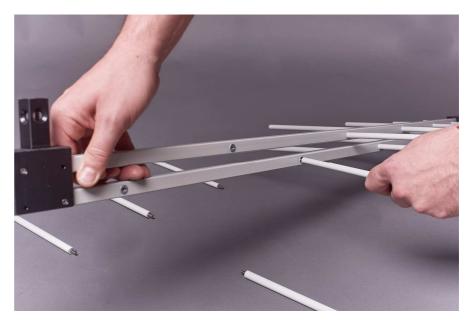





Assembly the 366mm length cylindrical dipole to the boom

Screw the two longer cylindrical dipole (449.5mm length) to the boom





Assembly the two triangle dipole to the boom unscrewing the knob from the threaded insert.





Mounting Instruction 2-5




Insert the triangle dipole on the threaded insert; position and rotate the dipole in order to the two metallic plugs and fix it into the boom by the knob.







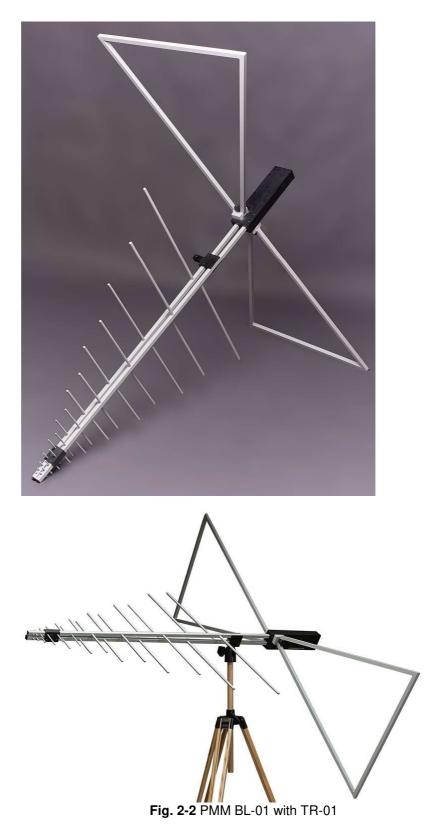



For further information on configuration and operation with PMM 9060, please refer to the operation manual supplied with it.



2.8 PMM LP-02 Log Periodic Dipole Array Screw the radiating elements on the main body of the LOG PERIODIC Antenna, choosing the radiating elements couple of equal length.

The antenna is composed by a total of 44 elements, only the longer 14 elements are removable.

Start screwing the shortest couple on the front side of the antenna, going on installing growing length elements on the connector side.





Unscrew the knob without to loose it completely.



Insert the tripod joint on the adjustable joint.



Change the antenna polarization from horizontal to vertical or vice versa and tighten the knob completely.



Fig. 2-3 PMM LP-02 with TR01



For further information on configuration and operation with PMM 9060, please refer to the operation manual supplied with it.



2.9 PMM LP-03 Log Periodic Dipole Array

The LP03 combines small size with high manufacturing and calibration standards, making it perfectly suitable for portable applications and in anechoic chambers.

The booms and the elements are made of aluminium Alodyne coated and painted; the holding pipe is made of stainless steel; the antenna is composed by a total of 28 elements.

Fix the adjustable joint to the TR01.



Remove the screws from the tripod joint.



Insert the LP-03 on the tripod joint and tighten the two screws to fix the LP-03 to the tripod join.



Mounting Instruction 2-9



Unscrew the knob without to loose it completely.



Insert the tripod joint on the adjustable joint.



Change the antenna polarization from horizontal to vertical or vice versa and tighten the knob completely.



Fig. 2-4 PMM LP-03 with TR01



For further information on configuration and operation with PMM 9060, please refer to the operation manual supplied with it.

2-10 Mounting Instruction



2.10 PMM LP-04 Log Periodic Dipole Array

Screw the radiating elements on the main body of the LOG PERIODIC Antenna, choosing the radiating elements couple of equal length.

The antenna is composed by a total of 2×18 elements, only the longer 2×3 elements are removable.

Start screwing the longest couple on the connector side of the antenna, going on installing the shorter length elements.





Unscrew the knob without losing it completely.



Insert the tripod joint on the adjustable joint.

Set the antenna polarization desired and tighten the knob completely.





For further information on configuration and operation with PMM 9060, please refer to the operation manual supplied with it.

Mounting Instruction 2

2-11



This page has been left blank intentionally



3 - Radiated Emission and Immunity testing

3.1 Radiated Emission The electromagnetic emissions emanating from the equipment under test testing (EUT) are measured during a radiated emission test According to the international Standards, the purpose of this test is to verify that the EUT's emissions are below specified limits during operation. The receiving antenna middle point can be located either at 3 or 10 meter from the EUT and must scan from 1 to 4 meters in height. This scanning helps the operator to locate the EUT's worst case electromagnetic emission level. The typical emissions test set-up is composed of: receive antenna; interconnecting cable; preamplifier; preamplifier cable; meter receiver. 3.1.1 The Antenna Factor The performance of the antenna relating to the value of the incident's field to the voltage output of the antenna is the Antenna Factor; this value is provided in dB/m by the manufacturer. 3.1.2 The The cable connects the antenna to the preamplifier or meter receiver input. There is a loss in the cable resulting in a reduction of the measured signal, interconnecting to increase the measure accuracy, these losses need to be added to the cable measured value. If the Receiver or the Spectrum Analyzer have a high input noise figure, 3.1.3 The preamplifier may be necessary to compensate it with a preamplifier installed between the antenna and the meter receiver. The preamplifier makes the measured signal larger, thus the gain of the preamplifier must be subtracted from the measured value to obtain the correct final result. 3.1.4 The preamplifier An additional cable to connect the preamplifier to the meter receiver input may be necessary if the preamplifier is installed. interconnecting There is a loss in the cable resulting in a reduction of the measured signal, cable to increase the measure accuracy, these losses need to be added to the measured value.

3-1



3.1.5 The meter receiver The meter receiver is typically either a radio receiver or a spectrum analyzer. Either a 120 kHz bandwidth and an output indication calibrated in dBµV are required.

The calculation of the measured E-field signal level is given by:

$$E\left(dB\frac{\mu V}{m}\right) = S\left(dB\mu V\right) + C_1\left(dB\right) - PA\left(dB\right) + C_2\left(dB\right) + AF\left(dB\frac{1}{m}\right)$$

where:

 $E\left(dB\frac{\mu V}{m}\right)$ =Corresponding Electric field

 $S(dB\mu V)$ = Measured signal strength

 $C_1(dB)$ = Preamplifier interconnecting cable

PA(dB) = Preamplifier gain

 $C_2(dB)$ = Interconnecting cable loss

$$AF\left(dB\frac{1}{m}\right)$$
 = Antenna factor

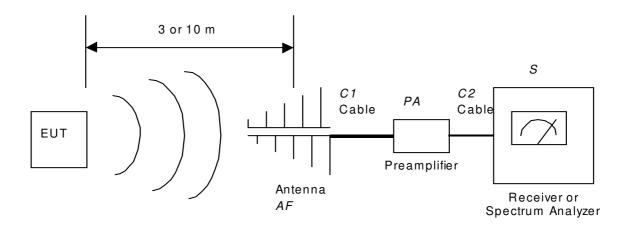


Fig. 3-1 Radiated emission test setup



3.2 Radiated Immunity testing	 During a radiated immunity test a electromagnetic signal, typically 3 or 10 V/m is directed at the equipment under test (EUT), analyzing the EUT reaction. According to the international Standards, the purpose of this test is to verify that the EUT does not show any degraded performance or failure when the signal is applied. The test should be performed either in horizontal and in vertical polarization. The transmitting antenna and the EUT are installed into a shielded room to avoid environmental RF pollution. A isotropic field probe must be located near the EUT to verify the electromagnetic field strength. The typical radiated test set-up is composed of: signal generator; power amplifier; transmit antenna; field strength meter. 				
3.2.1 The signal generator	The signal generator provides the test signal. It should have adequate output resolution to allow the setting of the field strength to within 1% of the desired level and must provide a sine wave 80% AM modulation at 1 kHz.				
3.2.2 The power amplifier	The power amplifier is used to increase the test signal strength applied to the antenna to a level able to produce the desired E-field. Note that the EMC amplifiers are specified with a minimum gain, they can show several dB of ripple in the pass band. The power amplifier must be operated in linear mode to assure repeatability, in fact when a 80% AM modulation is added an additional 5.1 dB $\left\{ 20x \log_{10}(1.8) \right\}$ of linear gain from the power amplifier is required.				
3.2.3 The transmit antenna	The performance of the antenna relating to the value of the emitted E-Field is the Antenna Factor. This is usually provided by the manufacturer in dB with units of inverse meters. Typically a combination of two antennas is used to cover the wide frequency range required by the Standard.				
3.2.4 The field strength meter	The field strength meter probe is used to directly measure the field level applied to the EUT. The typical distance between the tip of the antenna and the probe is 3 m.				



The calculation of the output level is given by:

$$E\left(dB\frac{\mu V}{m}\right) = G\left(dB\mu V\right) - C_1\left(dB\right) + A\left(dB\right) - C_2\left(dB\right) + TAF\Big|_{3m}\left(dB\frac{1}{m}\right)$$

where:

$$E\left(dB\frac{\mu V}{m}\right)$$
 =Generated Electric field

 $G(dB\mu V)$ = Signal Generator Level

 $C_1(dB)$ = Interconnecting cable loss

A(dB) = Power amplifier gain

 $C_2(dB)$ = Interconnecting cable loss

$$TAF|_{3m}\left(dB\frac{1}{m}\right) = \text{Transmit Antenna factor at 3 m} = 20\log_{10}(f_{MHz}) - AF|_{3m}\left(dB\frac{1}{m}\right) - 41,5$$

The variables and terms in the above expression are used for calibration test setup only. They demonstrate how the instrumentation and facility factors contribute to meet the typically required E-field uniformity value of -0.0 dB to + 6.0 dB.

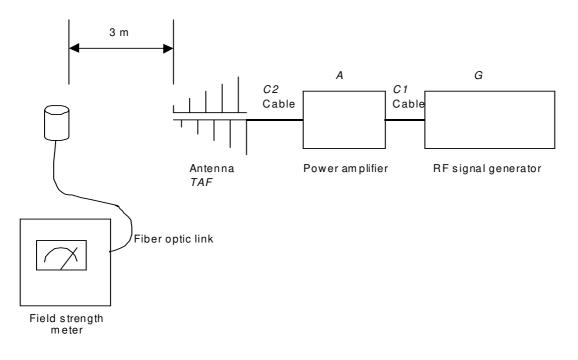


Fig. 3-2 Radiated immunity test setup



3.3 Environmental testing The PMM BC-01, BL-01, LP02, LP03, LP-04 and DR-01 antenna can also be used on environmental testing for narrow band electromagnetic field exposure testing. The wide frequency range and the low VSWR both allow accurate tests with linear polarization. For this kind of test the antenna must be used according to the following

For this kind of test the antenna must be used according to the following test setup, the receiver must have a good selectivity performance and must be tunable on the frequency or frequencies under investigation, a spectrum analyzer can be used instead.

The RF attenuator is normally installed as closest as possible to the antenna to improve the VSWR performances and then the precision of the measurement.

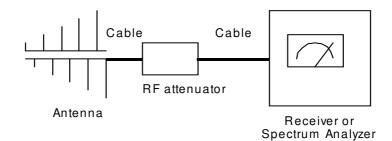


Fig. 3-3 Environmental test setup



This page has been left blank intentionally



 Manufa

 Via Ber

 17035

 Tel.: +3

 Unico

Manufacturing Plant: Via Benessea, 29/B 17035 - Cisano sul Neva (SV) Tel.: +39 0182 58641 Fax: +39 0182 586400

www.narda-sts.it nardait.support@narda-sts.it narda-sts@onlinepec.it



Caro cliente

grazie per aver acquistato un prodotto NARDA! Sei in possesso di uno strumento che per molti anni ti garantirà un'alta qualità di servizio. NARDA riconosce l'importanza del Cliente come ragione di esistenza; ciascun commento e suggerimento, sottoposto all'attenzione della nostra organizzazione, è tenuto in grande considerazione. La nostra qualità è alla ricerca del miglioramento continuo. Se uno dei Suoi strumenti NARDA necessita di riparazione o calibrazione, può aiutarci a servirla più efficacemente compilando questa scheda e accludendola all'apparecchio.

Tuttavia, anche questo prodotto diventerà obsoleto. In questo caso, ti ricordiamo che lo smaltimento dell'apparecchiatura deve essere fatto in conformità con i regolamenti locali. Questo prodotto è conforme alle direttive WEEE dell'Unione Europea (2002/96/EC) ed appartiene alla categoria 9 (strumenti di controllo). Lo smaltimento, in un ambiente adeguato, può avvenire anche attraverso la restituzione del prodotto alla NARDA senza sostenere alcuna spesa. Può ottenere ulteriori informazioni contattando i venditori NARDA o visitando il nostro sito Web www.narda-sts.it.

Dear Customer

thank you for purchasing a NARDA product! You now own a high-quality instrument that will give you many years of reliable service. NARDA recognizes the importance of the Customer as reason of existence; in this view, any comment and suggestion you would like to submit to the attention of our service organization is kept in great consideration. Moreover, we are continuously improving our quality, but we know this is a never ending process. We would be glad if our present efforts are pleasing you. Should one of your pieces of NARDA equipment need servicing you can help us serve you more effectively filling out this card and enclosing it with the product.

Nevertheless, even this product will become obsolete. When that time comes, please remember that electronic equipment must be disposed of in accordance with local regulations. This product conforms to the WEEE Directive of the European Union

(2002/96/EC) and belongs to Category 9 (Monitoring and Control Instruments). You can return the instrument to us free of charge for proper environment friendly disposal. You can obtain further information from your local NARDA Sales Partner or by visiting our website at <u>www.narda-sts.it</u>.

✓ Servizio richiesto:	✓ <u>Service needed</u> :					
		□ Riparazione & □ Repair & Calit		□ Taratura SIT □ Certified Calibration		Altro:] Other:
Ditta: <i>Company:</i>						
Indirizzo: Address:						
Persona da contattar Technical contact pers	-		Telefono: Phone n.			
Modello: Equipment model:						
Accessori ritornati con l'apparecchiatura:		<i>tura:</i> □ Nessuno □ None	□ Cavo(i) □ Cable(s)	□ Cavo di alimentazione □ Power cable		Altro: Other:
☑ <u>Sintomi o problem</u>	i osservati: ⊠ <u>Obs</u>	erved symptoms / pr	oblems:			
<i>☑ Guasto</i> : □ Fisso <i>☑ Failure</i> : □ Contir	□ Intermit nuous □ Intermit			□ Caldo □ Heat	□ Vibrazioni □ Vibration	□ Altro □ Other
Descrizione del guasto/condizioni di funzionamento: Failure symptoms/special control settings description:						
Se l'unità è parte di u If unit is part of system				set up:		

<u>Suggerimenti / Commenti / Note:</u> Suggestions / Comments / Note: